

# Fast Protein Quantification Assay kit (Bradford)

*KB-03-003*

*2000/4000 tests (96 well plate)*

# **BOCKit**

A brand of  BioQuoChem



# Index

---

<b>Introduction</b>	<b>Pag. 1</b>
<b>Materials</b>	<b>Pag. 2</b>
<b>Assay Principle</b>	<b>Pag. 3</b>
<b>Assay Protocol</b>	<b>Pag. 5</b>
<b>Data Analysis</b>	<b>Pag. 8</b>
<b>Warranties and Limitation of Liability</b>	<b>Pag. 9</b>



All chemicals should be handled with care

➤ **This kit is for R&D use only**

## *Introduction*

The Bradford assay, a colorimetric protein assay, is based on an absorbance shift of the dye Coomassie Brilliant Blue G-250.

Three charge forms of the Coomassie brilliant blue dye are present in equilibrium at the usual acidic pH of the assay. The red, blue, and green forms have absorbance maxima at 470, 590, and 650 nm, respectively.

The blue is the form that binds the protein, forming a complex that intensely absorbs light at 595 nm. During the formation of this complex, two types of bond interaction take place: the red form of Coomassie dye first donates its free electron to the ionizable groups on the protein, which causes a disruption of the protein's native state, consequently exposing its hydrophobic pockets. These pockets in the protein's tertiary structure bind non-covalently to the non-polar region of the dye via van der Waals forces, positioning the positive amine groups in proximity with the negative charge of the dye. The bond is further strengthened by the ionic interaction between the two.

The binding of the protein stabilizes the blue form of the Coomassie dye; thus the amount of the complex present in solution is a measure for the protein concentration, and can be estimated spectrophotometrically.

## Materials

BQCKitFast Protein Quantification kit **KB03003-2000 tests** contains:

Product	Quantity	Storage
<b>Bradford Reagent</b>	1 bottle	RT
<b>Protein Standard*</b>	2 vials	4°C

\*This Reagent is stable during 10 days at Room Temperature and is shipped in these conditions. Once received is recommended to keep it at 4°C.

BQCKit Fast Protein Quantification kit **KB03003-4000 tests** contains:

Product	Quantity	Storage
<b>Bradford Reagent</b>	2 bottles	RT
<b>Protein Standard*</b>	4 vials	4°C

\*This Reagent is stable during 10 days at Room Temperature and is shipped in these conditions. Once received is recommended to keep it at 4°C.

## *Assay Principle*

The Bradford assay is based on the direct binding of Coomassie brilliant blue G-250 dye to proteins at arginine, tryptophan, tyrosine, histidine and phenylalanine residues. Anionic dye binds to these residues producing an absorbance maximum at 595 nm.

The dye interacts with the protein via van der Waals forces between the hydrophobic regions of the protein and the non polar region of the dye, and the electrostatic interaction between the negatively charged dye and positively charged amino groups of protein. The formation of the dye-protein complex takes about two minutes and remains stable for an hour, so the procedure is very fast and the time for trial is not limiting. The dye-protein complex has a high extinction coefficient, which makes the assay highly sensitive.

Highly alkaline buffers present interference but it can be countered running appropriate targets. Reagents as magnesium chloride, potassium, sodium, ammonium sulfate and ethanol have no effect on the assay.

The presence of large amounts of detergents has a high interference.

Reagents commonly used are listed in Table 1.

# Assay Principle

**Table 1. Reagents compatible with the kit protein assay when the standard procedure is used\***

Chapso, 10%	Octyl $\beta$ -thioglucopyranoside, 1%
Deoxycholic acid, 0.2%	PBS
DMSO, 5%	Phenol Red, 0.5 mg/mL
Dithioerythritol(DTE), 10 mM	PIPES, 0.2 M
Dithiothreitol (DTT), 10 mM	PMSF, 2 mM
Eagle's MEM	Potassium chloride, 2 M
Earle's salt solution	Potassium phosphate, 0.5 M
EDTA, 0.2 M	SB 3-10, 0.1%
EGTA 0.2 M	SDS 0.025%
Ethanol, 10%	Sodium acetate, pH 4.8, 0.2 M
Glucose, 20%	Sodium azide, 0.5%
Glycerol, 5%	Sodium bicarbonate, 0.2 M
Glycine, 0.1M	Sodium Carbonate, 0.1 M
Guanidine-HCl, 2M	Sodium Chloride, 2.5 M
Hank's salt solution,	Sodium citrate pH4.8 or6.4,0.2 M
HCl, 0.1M	Sodium Hydroxide, 0.1M
HEPES 0.1M	Sodium Phosphate, 0.5M
Imidazole 0.2M	Sucrose, 10%
Magnesium chloride	TBP 5mM
MES, 0.1M	TBS (25mM Tris, 0.15M NaCl,
Methanol 10%	pH 7.6), 0.5x
Modified Dulbecco's PBS	TCEP, 20mM
MOPS, 0.1M	Thio-urea, 1M
Triethanolamine, pH 7.8, 50mM	Tricine, pH 8, 50mM
Tris, 1M	Triton® X-100, 0.05%
Tris-glycine (25mM Tris, 192mM glycine)	Tween® 20, 0.01%
Tris-glycine-SDS (25mM Tris, 192mM glycine, 0.1% SDS), 0.5x	Urea, 4M

\*These concentration limits are compatible for macroassay, when microassay is used, concentration limits are 1/25 of the values in Table 1.

Note: This is not a complete compatibility chart. There are many substances that can affect different proteins in different ways. One may assay the protein of interest in deionized water alone, then in buffer with possible interfering substances.

## Assay Protocol

There are two protocols to perform the assay. The microassay is for samples with low protein concentrations. The 96 well plate assay is for those who wish to perform the Bradford assay in plate format.

If another format is required, extrapolate the volume of samples and reagents.

### **BQC Fast Protein Quantification Kit Micro assay (2 mL)**

1. Invert the Bradford Reagent a few times before use.
2. Preparation of standards: Refer to the Table 2 as a guide for diluting the protein standard. For the diluent, use the same buffer as in the samples.

**Table 2.** *Microassay Standard Dilutions*

Sample	Standard [mL]	Diluent [mL]	Protein [mg]
S1(Blank)	---	2	---
S2	0.05	1.95	0.25
S3	0.1	1.9	0.5
S4	0.2	1.8	1
S5	0.4	1.6	2
S6	0.6	1.4	3
S7	0.8	1.2	4
S8	1	1	5

3. Pipette 1 mL of each standard or unknown sample solution into separate clean test tubes.



## Assay Protocol

4. Add 1 mL of Bradford Reagent to each tube and vortex.
5. Incubate at room temperature for at least 5 min. Samples should not be incubated longer than one hour at room temperature.
6. Measure the absorbance of these standards, blanks and unknown samples at 595 nm.

### **BQC Fast Protein Quantification Kit Microplate**

1. Invert the Bradford Reagent a few times before use.
2. Preparation of standards: Refer to the Table 3 as a guide for diluting the protein standard. For the diluent, use the same buffer as in the samples.
3. Pipette 5  $\mu\text{L}$  of each standard or unknown sample solution into microplate wells.


**Table 3. Microplate Standard Dilutions**

Sample	Standard [ $\mu\text{L}$ ]	Diluent [ $\mu\text{L}$ ]	Protein [ $\mu\text{g}$ ]
S1(Blank)	---	200	---
S2	5	195	1.25
S3	10	190	2.5
S4	20	180	5
S5	40	160	10
S6	60	140	15
S7	80	120	20
S8	100	100	25

# Assay Protocol

4. Add 250  $\mu\text{L}$  of Bradford Reagent to each well and vortex using a microplate mixer.
5. Incubate at room temperature for at least 5 min. Samples should not be incubated longer than one hour at room temperature.
6. Measure the absorbance of these standards, blanks and unknown samples at 595 nm.

## Plate set up

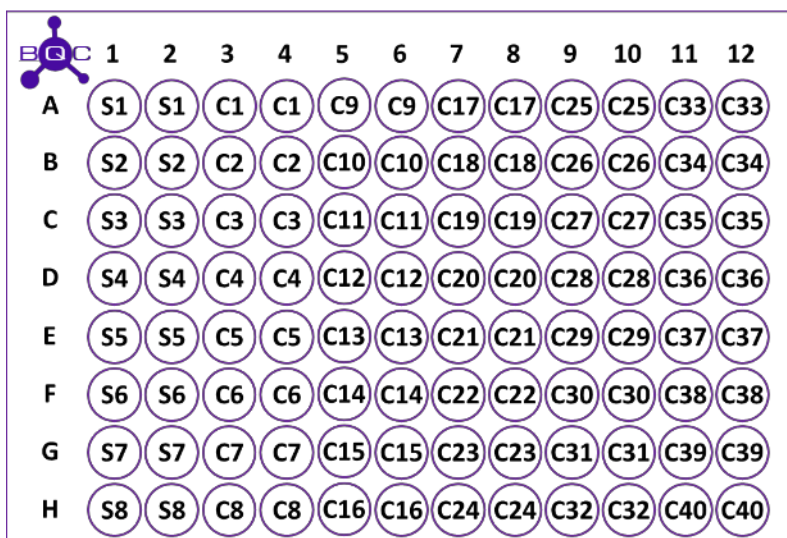


	1	2	3	4	5	6	7	8	9	10	11	12
A	S1	S1	C1	C1	C9	C9	C17	C17	C25	C25	C33	C33
B	S2	S2	C2	C2	C10	C10	C18	C18	C26	C26	C34	C34
C	S3	S3	C3	C3	C11	C11	C19	C19	C27	C27	C35	C35
D	S4	S4	C4	C4	C12	C12	C20	C20	C28	C28	C36	C36
E	S5	S5	C5	C5	C13	C13	C21	C21	C29	C29	C37	C37
F	S6	S6	C6	C6	C14	C14	C22	C22	C30	C30	C38	C38
G	S7	S7	C7	C7	C15	C15	C23	C23	C31	C31	C39	C39
H	S8	S8	C8	C8	C16	C16	C24	C24	C32	C32	C40	C40

### Attention

- This scheme is just a recommendation of how to perform the assay.
- For optimal results, it is recommended to run the standards and the samples for duplicate, but it is the user's discretion to do so.

## Data Analysis

1. If the spectrophotometer or microplate reader was not zeroed with the blank, then average the blank values and subtract the average blank value from the standard and unknown sample values.
2. Create a standard curve by plotting A 595 nm (y-axis) vs. standard,  $\mu\text{g}$  (x-axis). Determine the unknown sample concentration using the standard curve.
3. The level of detection of the assay is lower for the microplate assay when compared with the microassay due to a shorter light path used in the microplate reader.
4. Standard curve example for microplate assay procedure is shown in Figure 2.
5. Measure the absorbance of these standards, blanks and unknown samples at 595 nm.

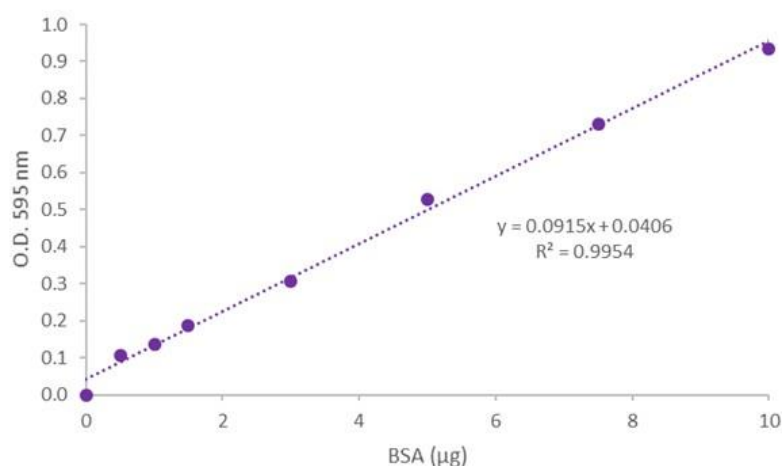

**Figure 2.** Typical standard curve for Bradford assay

## *Warranties and Limitation of Liability*

Bioquochem shall not in any event be liable for incidental, consequential or special damages of any kind resulting from any use or failure of the products, even if Bioquochem has been advised of the possibility of such damage including, without limitation, liability for loss of use, loss of work in progress, down time, loss of revenue or profits, failure to realize savings, loss of products of buyer or other use or any liability of buyer to a third party on account of such loss, or for any labor or any other expense, damage or loss occasioned by such product including personal injury or property damage is caused by Bioquochem's gross negligence. Any and all liability of Bioquochem hereunder shall be limited to the amounts paid by buyer for product.

Buyer's exclusive remedy and Bioquochem's sole liability hereunder shall be limited to a refund of the purchase price, or the replacement of all material that does not meet our specifications.

Said refund or replacement is conditioned on buyer giving written notice to Bioquochem within 30 days after arrival of the material at its destination.

Expiration date: 1 year from the date of delivery

For further details, please refer to our website [www.bqckit.com](http://www.bqckit.com).