


CERTIFICATE OF ANALYSIS



CUPRAC Assay Kit

Kit code: KF01005
Batch N°: 10050301
Expiry date: 03/January/2023
Standard calibration
Absorbance 450 nm 450 nm
Slope 1.194
R² 0.991

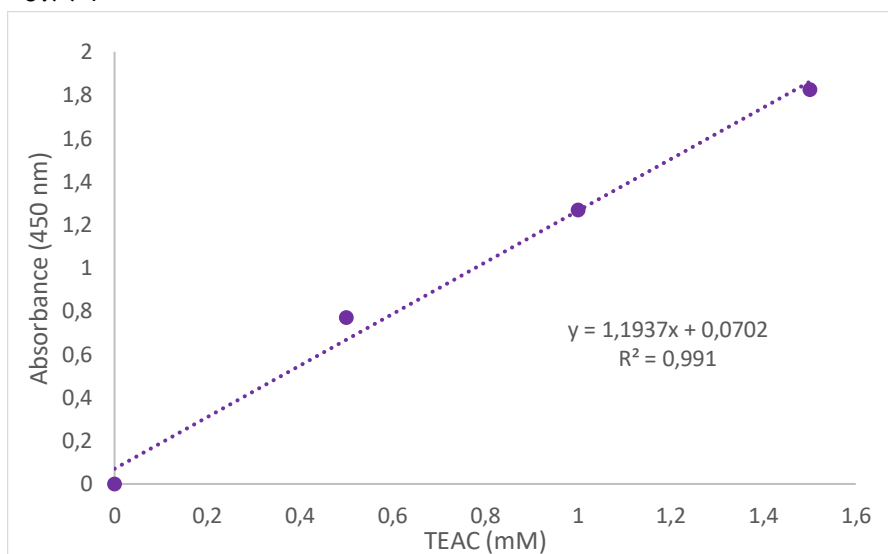

QUALITY CONTROL DEPARTMENT

BIOQUOCHEM S.L.

B - 74.389.386

Parque Tecnológico de Asturias
Edificio CEFI · 33428 Uanera